

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification <sup>6</sup> : <b>G01N 15/12, 1/38</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 98/22797</b> (43) International Publication Date: 28 May 1998 (28.05.98)</p>
<p>(21) International Application Number: PCT/SE97/01923 (22) International Filing Date: 17 November 1997 (17.11.97) (30) Priority Data: 9604259-3 20 November 1996 (20.11.96) SE (71) Applicant (for all designated States except US): MEDONIC AB [SE/SE]; Adolfsbergsvägen 13, S-168 66 Bromma (SE). (72) Inventors; and (75) Inventors/Applicants (for US only): BERNDTSSON, Ingemar [SE/SE]; Borevägen 9, S-191 43 Sollentuna (SE). ANDERSSON, Tommy [SE/SE]; Härjedalsgatan 20, S-162 66 Vällingby (SE). BOTTEMA, Abraham [NL/SE]; Stangvägen 13, S-148 71 Sorunda (SE). (74) Agents: SÄFWENBERG, Björn et al.; Axel Ehmers Patentbyrå AB, P.O. Box 10316, S-100 55 Stockholm (SE).</p>		<p>(81) Designated States: BR, CA, JP, US, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published With international search report.</p>

(54) Title: DILUTING AND MEASURING DEVICE FOR PARTICLE COUNTING

(57) Abstract

A device for particle counting includes means (21) for metering a volume of a liquid sample containing particles and a cylinder (33) for dosing a volume of a diluting liquid to a dilution chamber (72). The cylinder (32) has first and second ends and a piston (33). A conduit (18) connects a first end of the cylinder and the dilution chamber (72). The metering means (21) introduces the liquid sample in the conduit (18) and movement of the piston (33) towards the first end displaces diluting liquid and sample to the dilution chamber (72) which communicates with the second end of the cylinder (33) and is preferably located therein, whereby movement of the piston (33) towards the second end causes pressurising of the dilution chamber to displace diluted sample from the dilution chamber through a particle counting means (73). The piston (33) has a piston rod (34) extending through the first cylinder end, whereby movement of the piston towards the first end causes an increase in volume ( $V_2$ ) in the cylinder on the second piston side that is greater than the decrease in volume ( $V_1$ ) in the cylinder on the first piston side. The increase causes a lowered pressure on the second piston side that draws air into the dilution chamber.

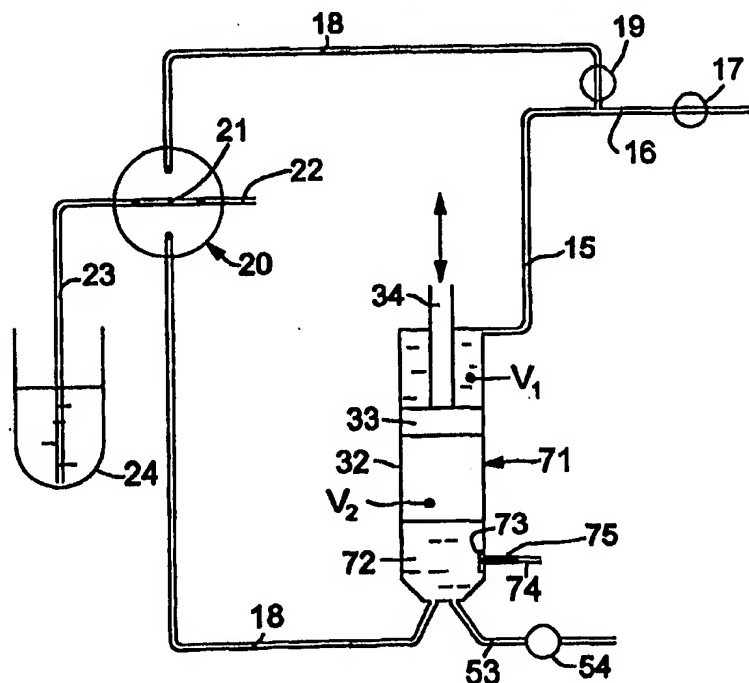

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece		Republic of Macedonia	TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CJ	Côte d'Ivoire	KP	Democratic People's	NZ	New Zealand		
CM	Cameroon		Republic of Korea	PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

## DILUTING AND MEASURING DEVICE FOR PARTICLE COUNTING

The present invention concerns a diluting and measuring device for particle counting according to the preamble of claim 1.

5 This device is particularly, but not exclusively, intended for the counting of blood cells.

It is known in the state of the art to count blood cells by causing an accurately defined volume of diluted blood sample to  
10 pass a so-called capillary, i.e., an extremely small hole, generally in a ruby, the hole having a diameter considerably larger than the size of a blood cell, typically 80 $\mu$ m. A voltage is applied over the capillary, and, when a blood cell passes through the hole, the electrical resistance changes. This is  
15 because the cells can be regarded as insulators. Each change in resistance can be detected by suitable electronic equipment, and the sum of all changes detected corresponds to the number of blood cells having passed through the capillary. In order to obtain the concentration of cells in the original sample, the  
20 concentration of cells in the diluted sample is multiplied by the dilution factor, typically 1:40000 when counting of red blood cells (RBC) is concerned. It is obvious, that measuring of sample volumes and dilution liquid volumes must be performed in an accurate and repeatable way such that not only a correct  
25 degree of dilution can always be guaranteed but also a thorough and uniform mixing of the two volumes is ensured.

In a typical state of the art apparatus, a syringe is employed for providing a defined volume (typically 5 ml) of diluting  
30 liquid, and this volume is displaced through a conduit to a measuring chamber. On its way to the measuring chamber, the diluting liquid brings with it a defined volume (typically 25  $\mu$ l) of blood sample previously introduced into the conduit. The blood sample mixes with and is diluted by the diluting  
35 liquid in the measuring chamber, which is, thus, also a dilution or mixing chamber, and a defined fraction of the diluted sample is further displaced through a capillary located

in a wall of the measuring chamber, or, in a transducer located within the measuring chamber.

5 This state of art apparatus requires a syringe for the diluting liquid and a separate mixing/measuring chamber. It would be desirable, thus, to simplify the apparatus by combining the syringe and at least a mixing chamber.

10 Also, in this state of art apparatus, the mixing between the blood sample and the diluting liquid in the measuring chamber is caused by turbulence when the two liquids enter the measuring chamber and cannot be enhanced in any way. It would be desirable, thus, to enhance the turbulence in the mixing chamber, thereby to reach a more uniform mixing of the sample  
15 and the diluting liquid. One known method to achieve turbulence in a liquid is to let air bubbles into a mixing chamber at the bottom thereof by means of a pump. Evidently, the need of a pump makes the apparatus more expensive and cumbersome and increases the need of maintenance.

20 The present invention has as its object to provide, on one hand, a possibility to combine a dosing syringe and a mixing chamber that may also be a measuring chamber, and on the other hand a means to enhance the mixing in a mixing chamber between  
25 a sample containing particles at a relatively high concentration and a diluting liquid by introducing air into the mixing chamber without the need for a pump or the like.

To achieve these objects, the present invention suggests, on  
30 one hand, to utilize the volumes of a syringe on either sides of its piston, on a first side for receiving and dispensing diluting liquid and on a second side for providing a mixing chamber that may be combined with a measuring chamber.

35 On the other hand, the present invention suggests introducing air at the bottom of the mixing chamber by lowering the pressure in the mixing chamber, so that air is sucked into the

mixing chamber. Advantageously, a piston of the dosing syringe used for dosing the diluting liquid is also utilized for lowering the pressure in the mixing chamber. Preferably, the piston has a first side having a relatively small area for dosing the diluting liquid, and a second side having a relatively large area, so that a defined displacement of the piston in the dosing direction causes displacement of a defined volume of diluting liquid and an increase in volume on the second side of the piston that is greater than said defined volume. This, in turn, creates a lowered pressure in an air volume on the second side of the piston which is used to suck air into the mixing chamber.

Embodiments of the present invention will be described hereinafter, reference being made to the annexed drawings, wherein:

- Fig. 1 is a schematic view showing a state of the art apparatus;
- 20 - Fig. 2 is a schematic view showing a second embodiment of the present invention employing a combined mixing and measuring chamber separate from a syringe;
- Fig. 3 is a schematic view showing a first embodiment of the present invention employing a mixing chamber integrated in a syringe and a separate measuring chamber;
- 25 - Fig. 4 is a schematic view showing a fourth embodiment of the present invention employing a combined mixing and measuring chamber integrated in a syringe; and
- Fig. 5 is a schematic view showing a fifth, preferred embodiment of the present invention employing a combined mixing and measuring chamber integrated in a syringe.
- 30

In the state of art arrangement according to Fig. 1, 11 is a syringe including a cylinder 12 and a piston 13 axially movable within the cylinder by means of a piston rod 14 extending through one end of the cylinder, that may be an open end. The opposite end of the cylinder is closed and connected to a

conduit 15. This conduit 15 in turn communicates with a supply conduit 16 for diluting liquid having a valve 17 therein, and a discharge conduit 18 having a valve 19 therein. In the conduit 18 there is also a turning valve 20, the non-shown rotatable valve body of which has a through channel 21 and is positionable in two different positions. In a first position (shown in Fig. 1), the through channel communicates with a conduit 22 leading to a non-shown pump, and a conduit 23 communicating with a vessel 24 containing a blood sample to be diluted. The blood sample in the vessel 24 may be diluted already to a certain extent. The discharge conduit 18 ends in a mixing and measuring chamber 25. Upon operation of the pump, blood sample is transported from the vessel 24 through the valve 20 so as to fill the through channel 21. In a second position of the valve body, the through channel communicates with the conduit 18. Since the through channel 21 contains an accurately defined volume, turning of the valve body to the second position will put this defined volume in communication with the conduit 18.

The function of the known device is as follows: The valve 17 is opened and the piston lowered to suck a defined volume of diluting liquid into the syringe. Thereafter, the valve 17 is closed and the valve 19 opened, and the piston 13 is raised thereby displacing diluting liquid through the conduit 18 through the valve 20, the valve body of which being positioned in its second position so that the defined volume of blood sample is brought by the diluting liquid to the mixing and measuring chamber 25 where the very small volume of blood sample is to be mixed with and diluted by the relatively large volume of diluting liquid. In a wall of the chamber 25 there is a capillary 26 and a discharge conduit 27.

It is evident that the only mixing occurring in the chamber 20 is due to turbulence when the sample and the diluting liquid enter the chamber.

To improve the mixing of the sample and the diluting liquid, the present invention provides for admission of air into the chamber without the need for a pump or the like.

5 In Fig. 2, reference numerals 15 - 24 are used to designate items corresponding to those of Fig. 1. The syringe of Fig. 1 is replaced by a syringe 31 including a substantially vertical cylinder 32 having a double-acting piston 33 axially movable therein by means of a piston rod 34 attached to one side of the  
10 piston and sealingly extending through a closed end of the cylinder. The interior of this end of the cylinder communicates with the conduit 15. The opposite, lower end of the cylinder, which is likewise closed, communicates with a combined mixing and measuring chamber 35 through a conduit 36 opening in an  
15 upper closure 37. The discharge conduit 18 for diluting liquid extends through the closure and opens within the chamber 35. In a wall of the chamber is a capillary 38 and a discharge conduit 39 including a metallic portion 40 constituting an electrode connected to an electric wire 41. A further electrode 42 is  
20 located within the chamber 35 and is connected to an electric wire 43. At the bottom of the chamber 35 there is a conduit 44 having a valve 45. Also the conduit 44 may have a metallic portion 46 constituting an electrode connected to an electric wire 47. A voltage may be applied across the capillary by  
25 connecting wire 41 to one pole and either or both of wires 43, 47 to the other pole of a suitable electronic counting equipment.

The function of the apparatus of Fig. 2 is as follows: Valve 19  
30 is closed and valve 17 opened and the piston rod 34 is operated to lower the piston a predetermined distance from its upper position. A diluting liquid, typically an isotonic solution of NaCl when dilution of a blood sample and counting of RBC is concerned, is drawn from a non-shown source into the upper  
35 volume  $V_1$  of the syringe 31 through conduits 16 and 15. Thereafter, valve 17 is closed and valve 19 opened, and the valve body of turning valve 20 is rotated so as to connect its

through channel 21 to conduit 18. Now the piston rod 34 is operated to raise the piston 33 thereby displacing the diluting liquid through conduits 15 and 18 and bringing along the blood sample from the through channel 21 to the chamber 35.

5 Simultaneously, the lower volume  $V_2$  of the syringe increases more than the upper volume  $V_1$  decreases due to the larger effective piston area on the lower side of the piston. This leads to a lowering of the pressure in an air volume in the lower volume  $V_2$ . Now the valve 45 is opened and air under  
10 atmospheric pressure is allowed to enter the conduit 44 and the chamber 35 at its bottom to create at least one air bubble raising through the mixture of blood sample and diluting liquid therein creating further turbulence than was the result of the mere introduction of the sample with the diluting liquid. This  
15 results in the desired enhanced mixing and, as a consequence, a more uniform distribution of the blood cells within the volume.

The embodiment of Fig. 3 differs from that of Fig. 2 in that a mixing chamber is integrated in the syringe 51, simply by  
20 employing the lower volume  $V_2$  as a mixing chamber 52 into which open the conduit 18 as well as an air inlet conduit 53 having a valve 54. A conduit 55 leads from the chamber 52 to a separate measuring chamber 56 having a capillary 57, a discharge conduit 58 as well as electrodes 59 and 60 with electric wires 61, 62,  
25 respectively. Whereas the entire lower volume  $V_2$  was dry in the embodiment of Fig. 2, it will contain in Fig. 3 an upper air volume and a lower volume of blood sample and diluting liquid once the piston has been raised to displace the diluting liquid. As before, the differential in areas of the upper and  
30 lower sides of the piston causes lowering of the pressure in the lower volume  $V_2$  which is used to draw air into the mixing chamber 52 upon opening of the valve 54.

The embodiment of Fig. 4 differs from that of Fig. 3 in that  
35 the syringe 71 employs its lower volume  $V_2$  as a mixing and measuring chamber 72. Thus, the only difference in comparison to Fig. 3 is that a capillary 73 is located in the wall of the



syringe and has a discharge conduit 74 with an electrode 75. At least one further electrode is arranged as a metallic portion of conduit 18 and/or conduit 53 (not shown).

- 5 Fig. 5 shows a preferred embodiment of a syringe 81 having a combined mixing and measuring chamber 82. Here, the conduit 18 for introduction of the sample and the diluting liquid into the chamber 82 describes a substantially vertical loop 83 before its end is connected to the bottom end of the syringe. The loop
- 10 includes a V-shaped portion having a first leg 84 and a second leg 85. At the bottom of the V-shape the conduit 18 communicates with a capillary 86 located in the wall of the syringe. The conduit 18 has a further valve 87 between the loop and the syringe. At the bottom of the syringe there may be an
- 15 emptying conduit 88 with a valve 89 (such conduit and valve may be provided on the syringes previously described as well). At least one electrode is provided on each side of the capillary, suitably by metallic portions of the conduits connected to the syringe. In order to reduce the influence of air bubbles
- 20 possibly adhering to the inner sides of the conduits, it is preferred, however, that two electrodes are provided on each side. Thus, one electrode 90 is arranged on the leg 84 and one electrode 91 is arranged on the leg 85 of the conduit 18. An electric wire 92 connects electrodes 90 and 91, and electric
- 25 wire 93 leads away from electrode 91. Correspondingly, one electrode 94 is arranged on the conduit 18 between the valve 87 and the syringe, and one electrode 95 is arranged on the conduit 53 between the syringe and the valve 54. An electric wire 96 connects electrodes 94 and 95, and an electric wire 97
- 30 leads away from electrode 95. In order to prevent short-circuiting between the electrodes 90, 91 and 94, 95 the valve 87 has an insulating function in its closed position. A branch conduit 98 leads away from the conduit 18 and has a valve 99.
- 35 In operation of the embodiment of Fig. 5, the diluting liquid and blood sample displaced by the piston 33 through the conduit 18 passes the loop 83 before entering the chamber 82. In

passing the legs 84 and 85 of the loop, the liquid will flush away air bubbles possibly adhering to the inner sides of the legs 84, 85, particularly the portions thereof serving as electrodes. At this stage the valve 87 is open and the valve 99  
5 closed as are the valves 54 and 89. Due to the very small opening of the capillary 86, only a neglectible volume of the liquid will enter the chamber 82 through the capillary.

When the predetermined volume has entered the chamber 82, the  
10 valve 54 is opened to introduce air into the chamber 82 for mixing the blood sample with the diluting liquid. Thereupon the valve 54 is closed, the valve body of the turning valve 20 is brought to the position shown blocking conduit 18, the valve 87 is closed and the valve 99 is opened. The piston 33 is  
15 lowered to press the diluted sample through the capillary 86 and the leg 84 of the loop 83 into the conduit 18 from where it enters the conduit 98. In the conduit 98 there is a transparent portion having two light sensors 100 and 101 spaced therealong a distance 102 corresponding to a predetermined volume within  
20 the conduit 98. These sensors will sense a change in the refractive index of the liquid passing them. Since the conduit 18 will be filled with only clear diluting liquid after having displaced the volume of blood sample contained within the through channel 21 of the turning valve 20 through the conduit  
25 18 and into the chamber 82, the liquid first passing the sensors will be the transparent volume of diluting liquid contained in the portion of the conduit 18 between the capillary 86 and the branching point between conduits 18 and 98. As soon as liquid having another refractive index, i.e.  
30 diluted blood sample, passes the first sensor, the blood cell counting starts, and as soon as the same change is indicated at the second sensor, the counting stops. The result obtained is the number of blood cells contained within the defined volume (typically 200 - 400  $\mu$ l) between the sensors 100 and 101, and  
35 this number is divided by the predetermined volume to obtain the concentration in the sample. It is now easy to determine

the concentration of blood cells in the original, undiluted blood sample by multiplying by the dilution factor.

## CLAIMS

1. A diluting and measuring device for particle counting, including metering means (21) for metering a defined volume of a liquid sample containing particles, dosing means (31; 51; 71; 81) for dosing a defined volume of a diluting liquid for diluting said defined volume of said sample, and a dilution chamber (35; 52; 72; 82), said dosing means including a cylinder (32) having a first and a second end and a piston (33) axially movable in said cylinder and having a first and a second piston side,  
c h a r a c t e r i z e d   b y
- first conduit means (18) connecting said first end of said cylinder and said dilution chamber (35; 52; 72; 82), said metering means (21) being adapted to introduce said defined volume of said liquid sample in said first conduit means (18), whereby movement of said piston (33) towards said first end causes displacement of said defined volume of said diluting liquid through said first conduit means (18) to said dilution chamber (35; 52; 72; 82), thereby bringing along said defined volume of said sample to be diluted by said diluting liquid in said dilution chamber;
  - said dilution chamber (35; 52; 72; 82) communicating with said second end of said cylinder (32), whereby movement of said piston (33) towards said second end causes pressurising of said dilution chamber to displace diluted sample from said dilution chamber through a particle counting means (38; 57; 73; 86) communicating with said dilution chamber.
2. A particle counting device according to claim 1, c h a r a c t e r i z e d   i n   t h a t said particle counting means (38; 57; 73; 86) is located in a wall of said dilution chamber (35; 52; 72; 82) which is also a measuring chamber.
3. A particle counting device according to claim 1, c h a r a c t e r i z e d   i n   t h a t said particle counting

means (57) is located in a wall of a separate measuring chamber (56) communicating with said dilution chamber (52).

4. A particle counting device according to claim 1 or 2,  
5 c h a r a c t e r i z e d i n t h a t s a i d d i l u t i o n c h a m b e r  
(52; 72; 82) comprises said second end of said cylinder (32).

5. A particle counting device according to claim 4,  
c h a r a c t e r i z e d i n t h a t s a i d f i r s t c o n d u i t m e a n s  
10 (18) describes a substantially vertical loop (83) connected to  
said cylinder (32) such that the interior of the cylinder on  
said second piston side ( $V_2$ ) communicates with said first  
conduit means (18) through said particle counting means (86).

15 6. A particle counting device according to claim 5,  
c h a r a c t e r i z e d i n t h a t s a i d l o o p (83) includes a  
first (84) and a second leg (85) joined in a position where  
said first conduit means (18) is connected to said cylinder  
(32), that said first leg (84) ascends towards said position  
20 and said second leg (85) ascends from said position, and that  
at least one of said legs (84,85) includes an electrically  
conducting portion (90,91) constituting first electrode means  
electrically connected to liquid within said first conduit  
means (18).

25 7. A particle counting device according to claim 6,  
c h a r a c t e r i z e d i n t h a t a t l e a s t o n e s e c o n d  
electrode means (94,95) is provided being electrically  
connected to liquid within said cylinder on said second piston  
30 side ( $V_2$ ).


8. A particle counting device according to claim 7,  
c h a r a c t e r i z e d i n t h a t s a i d s e c o n d e l e c t r o d e  
means is constituted by an electrically conducting portion  
35 (94,95) of at least one second conduit means (53).

9. A particle counting device according to claim 1,  
c h a r a c t e r i z e d i n that said piston (33) is  
operable by means of a piston rod (34) connected to said first  
piston side and extending through said first cylinder end,  
5 whereby movement of said piston towards said first end causes  
an increase in volume ( $V_2$ ) in said cylinder on said second  
piston side that is greater than the decrease in volume ( $V_1$ ) in  
said cylinder on said first piston side, said increase causing  
a lowered pressure in an air volume on said second piston side,  
10 said cylinder being provided with means (44,45; 53,54; 88,89)  
for letting atmospheric air into said cylinder at its second  
end to equalize said lowered pressure.

10. A particle counting device according to claim 9,  
15 c h a r a c t e r i z e d i n that said means for letting  
atmospheric air into said cylinder opens in a lower portion of  
said dilution chamber (35; 52; 72; 82) located below a common  
liquid level of said defined volume of said diluting liquid and  
said defined volume of said sample contained within said  
20 dilution chamber.

1/5


Fig. 1

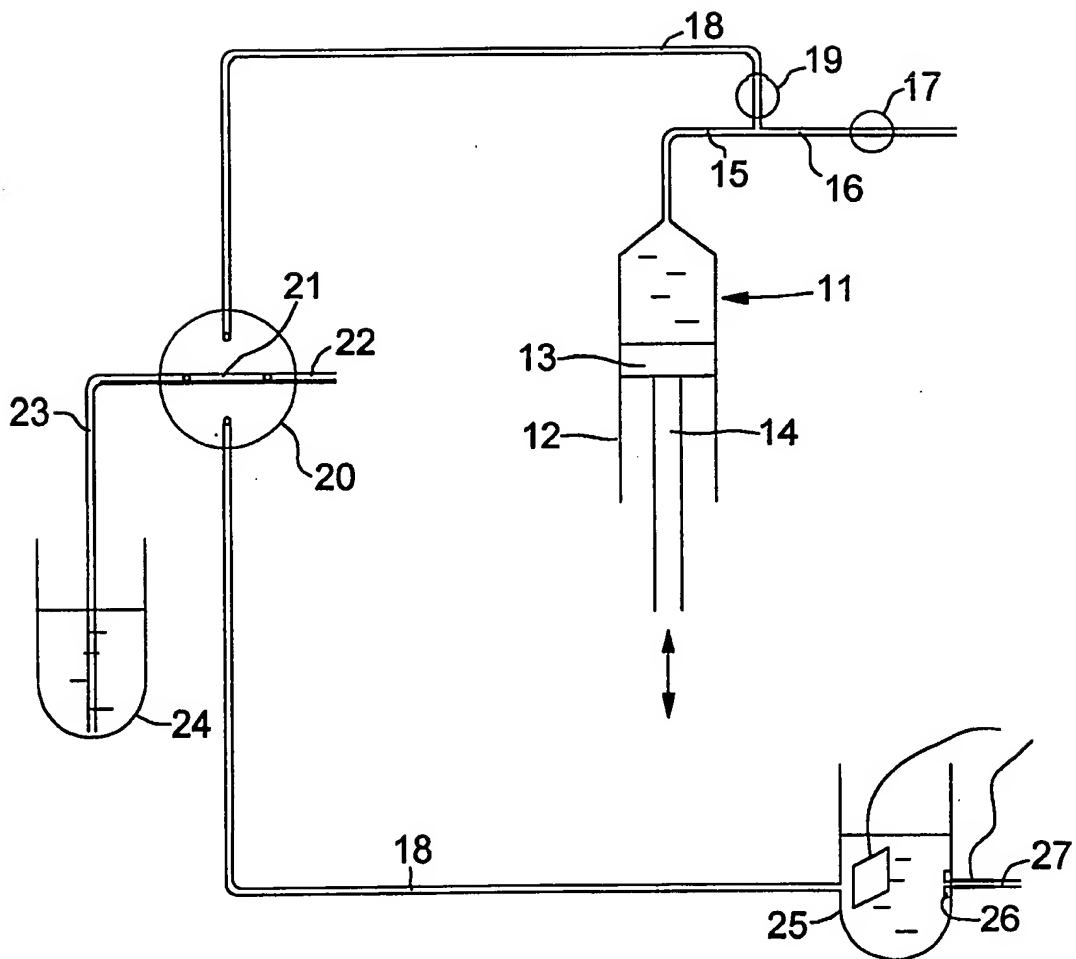

PRIOR ART

2/5


Fig. 2

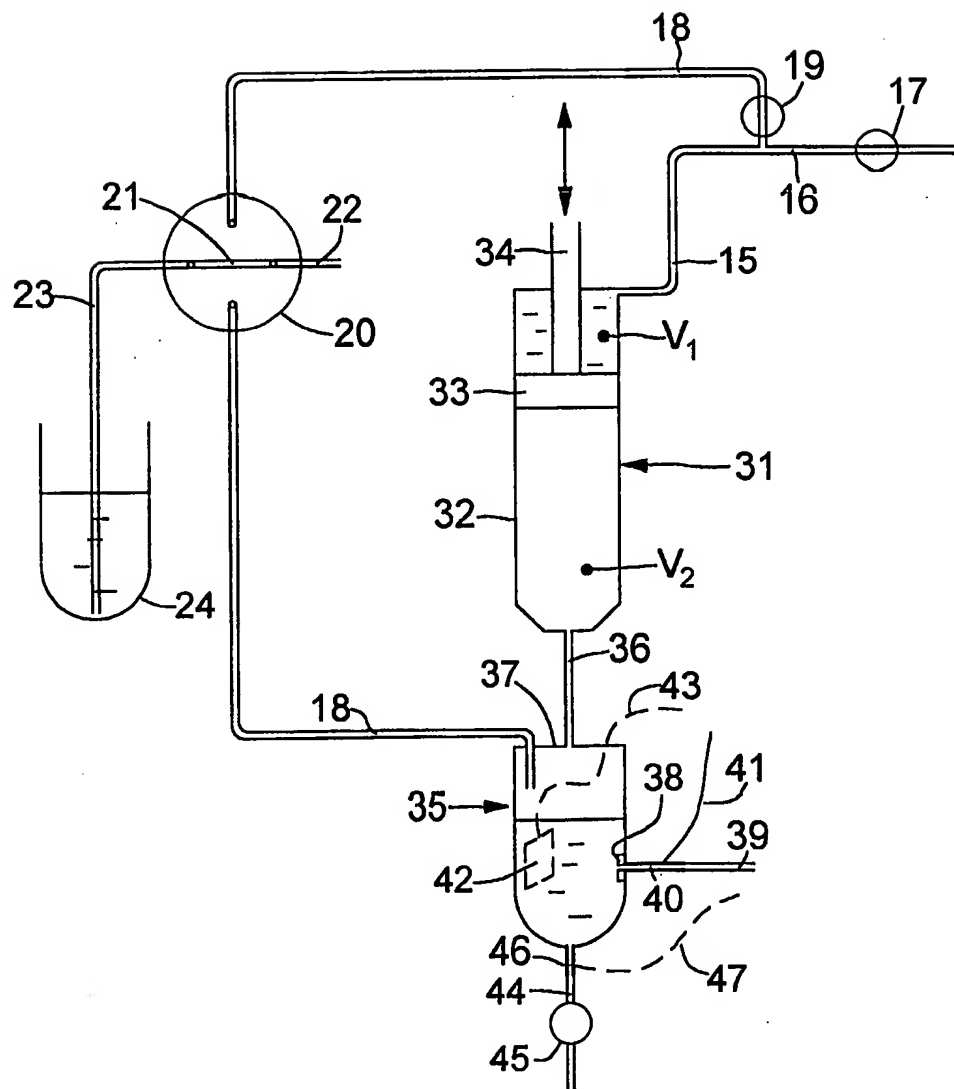




3/5

Fig. 3

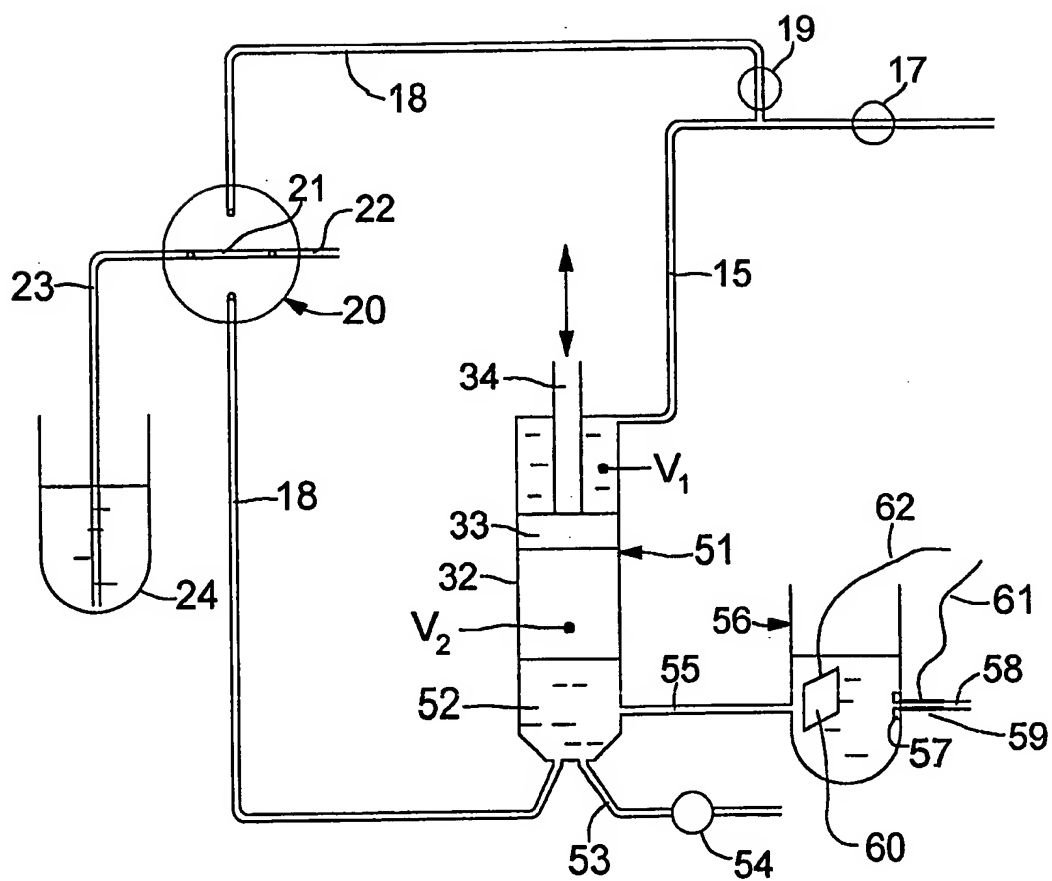


4/5

Fig. 4

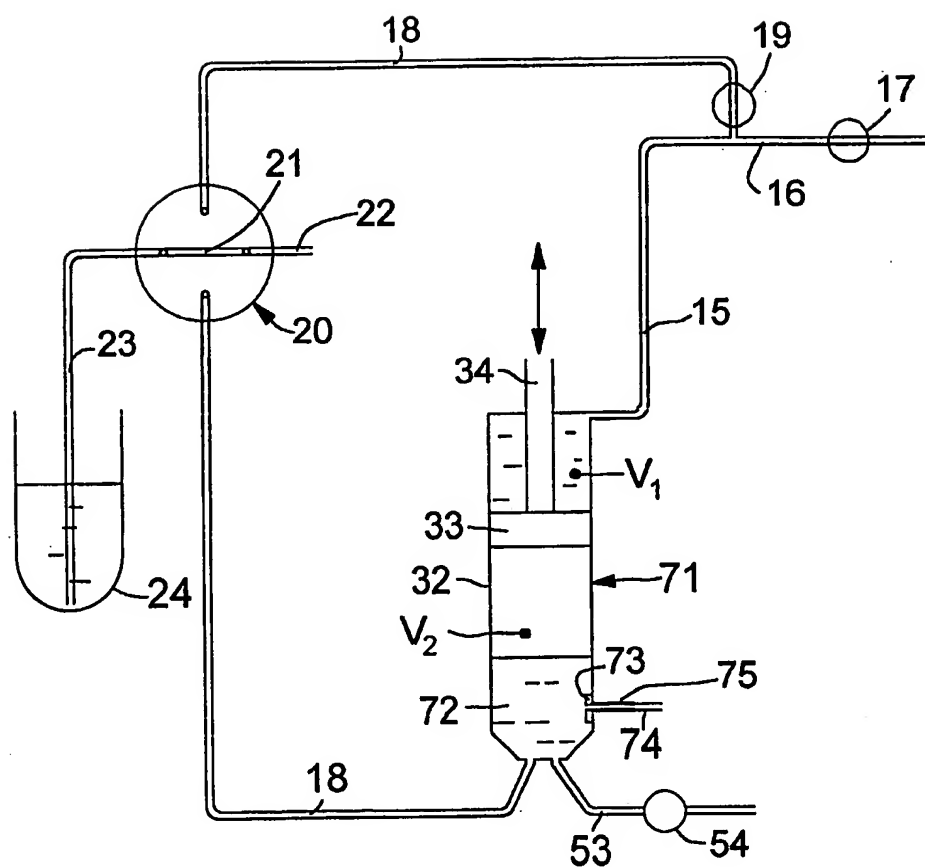

**5/5**

**Fig. 5**

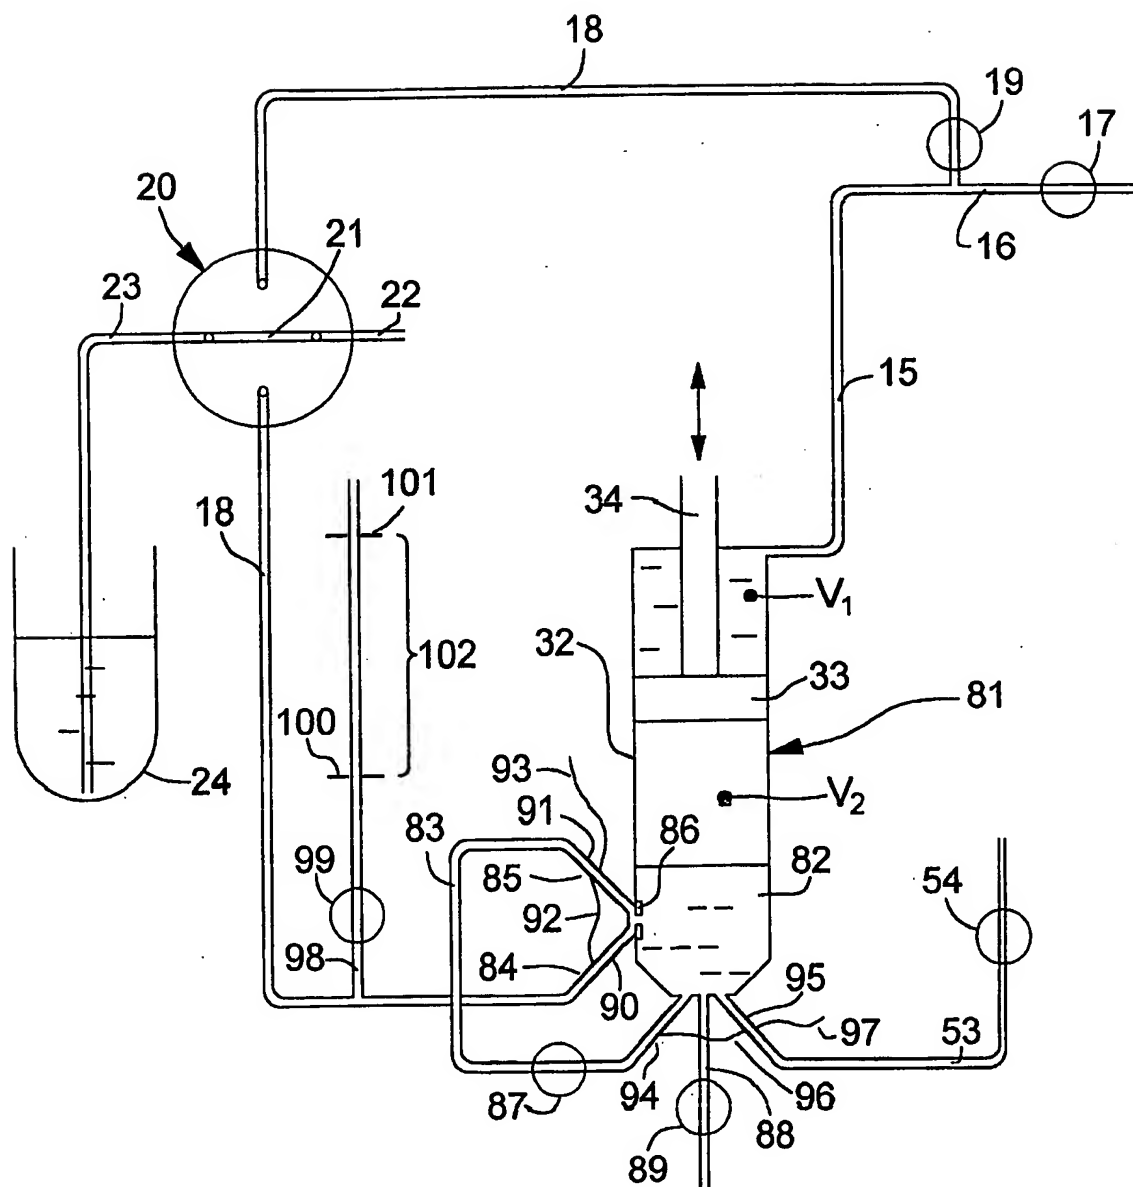

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 97/01923

## A. CLASSIFICATION OF SUBJECT MATTER

IPC6: G01N 15/12, G01N 1/38

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC6: G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

WPI, EPODOC

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	SE 456866 B (MEDONIC INGEMAR BERTSSON AB), 7 November 1988 (07.11.88) --	1-10
A	WO 9525269 A1 (COUNTING TECHNOLOGY LIMITED), 21 Sept 1995 (21.09.95) --	1-10
A	US 4090129 A (ADRIAN R.L.GEAR), 16 May 1978 (16.05.78) --	1-10
A	US 3496970 A (J.A. PONTIGNY), 24 February 1970 (24.02.70) --	1-10

☒ Further documents are listed in the continuation of Box C.☒ See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;" document member of the same patent family

Date of the actual completion of the international search

4 March 1998

Date of mailing of the international search report

09 -03- 1998

Name and mailing address of the ISA

Swedish Patent Office  
Box 5055, S-102 42 STOCKHOLM  
Facsimile No. +46 8 666 02 86

Authorized officer

Britt-Marie Lundell

Telephone No. +46 8 782 25 00

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 97/01923

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 3165693 A (J.ISREELI ET AL), 12 January 1965 (12.01.65)  -- -----	1-10

**INTERNATIONAL SEARCH REPORT**  
Information on patent family members

03/02/98

International application No.

PCT/SE 97/01923

Patent document cited in search report			Publication date	Patent family member(s)	Publication date
SE	456866	B	07/11/88	SE 8703897 A	07/11/88
WO	9525269	A1	21/09/95	EP 0750740 A	02/01/97
				GB 9405028 D	00/00/00
US	4090129	A	16/05/78	NONE	
US	3496970	A	24/02/70	FR 1475725 A	00/00/00
US	3165693	A	12/01/65	CH 415114 A	00/00/00
				DE 1214905 B	00/00/00
				FR 1325237 A	00/00/00
				GB 986978 A	00/00/00
				US 3165692 A	00/00/00